

University of Groningen

A New Data Acquisition System for the Groningen Counters

Plicht, Johannes van der; Streurman, H.J.; Schreuder, G.R.

Published in:
Radiocarbon

IMPORTANT NOTE: You are advised to consult the publisher's version (publisher's PDF) if you wish to cite from it. Please check the document version below.

Document Version
Publisher's PDF, also known as Version of record

Publication date:
1992

[Link to publication in University of Groningen/UMCG research database](#)

Citation for published version (APA):

Plicht, J. V. D., Streurman, H. J., & Schreuder, G. R. (1992). A New Data Acquisition System for the Groningen Counters. *Radiocarbon*, 34(3), 500-505.

Copyright

Other than for strictly personal use, it is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), unless the work is under an open content license (like Creative Commons).

The publication may also be distributed here under the terms of Article 25fa of the Dutch Copyright Act, indicated by the "Taverne" license. More information can be found on the University of Groningen website: <https://www.rug.nl/library/open-access/self-archiving-pure/taverne-amendment>.

Take-down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Downloaded from the University of Groningen/UMCG research database (Pure): <http://www.rug.nl/research/portal>. For technical reasons the number of authors shown on this cover page is limited to 10 maximum.

A NEW DATA ACQUISITION SYSTEM FOR THE GRONINGEN COUNTERS

JOHANNES VAN DER PLICHT, H. J. STREURMAN and G. R. SCHREUDER¹

Center for Isotope Research, University of Groningen, Nijenborgh 4
9747 AG Groningen, The Netherlands

ABSTRACT. A new GPIB/IEEE-488 based data acquisition system has been built for the Groningen proportional counter setup, consisting of 11 counters. The IEEE bus is connected to an XT-compatible host PC. A versatile computer program controls the data entry; the same program can be used offline for final calculations.

INTRODUCTION

The Groningen laboratory operates 11 proportional counters; 3 are used for tritium and 8 for radiocarbon. Three of the ^{14}C counters can be combined into one large high-precision counter. Table 1 summarizes the main properties of the Groningen counters. The counters are numbered 1–9; 3, 4 and 5 are the tritium counters, and 9 consists of the subsets A, B and C. The counter system developed for milligram-sized samples (Counter 10; Hut, Keyser & Wijma 1983) is not included; this setup was contaminated because of the Chernobyl accident, and is decommissioned.

Each counter system has its own amplifier (within the lead shielding close to the proportional counter) and discriminator unit. Until 1990, the discriminator units were read out by an ITT 2020 (Apple IIe compatible) microcomputer *via* a locally designed interface. Secondary parameters, such as counter gas pressures, temperatures and barometer reading were routed to the same microcomputer *via* a different locally designed interface. For the large counter (no. 9), not all parameters could be handled by the ITT2020 because of its limited memory (48 kb).

In 1990, we replaced the ITT2020 with an Olivetti M240 (XT-compatible) PC with an IEEE-based interface system. The discriminator units had to be rebuilt to incorporate the new standard. We also replaced the amplifiers with modern ones with better signal-to-noise ratios and completely rewrote the software for the new data acquisition system into Turbo Pascal.

THE COUNTERS

We use CO_2 as counting gas in the Groningen proportional counters for ^{14}C . As is well known, this requires a high degree of gas purity (Mook & Streurman 1983; Brenninkmeijer & Mook 1979). In routine CO_2 counter operation, the gas purity is determined in the counter itself. At fixed counting conditions (such as high voltage and pressure), electronegative impurities result in a decrease in pulse height; this causes a shift of the beta plateau toward higher voltages. A similar shift occurs in the meson characteristic curve, which is measurable by the decrease in counting rate at the steep part of the curve. The decrease in meson counting rate can be converted to that in the beta counting rate through a comparison of the respective slopes. The corrected count rate then becomes

$$A_c = A_m \left[1 - (N_z - N_{z_0}) \left(\frac{dV}{dN_\mu} \right)_{\max} \left(\frac{dN_\beta}{dV} \right)_{\text{recent}} A_o^{-1} \right] \quad (1)$$

¹Electronics Department, University of Groningen

TABLE 1. The Groningen Proportional Counters

Counter	No. of counters	Material	Volume (ml)	Pressure (mbar)	Min. amt. of C (g)	Max. age (BP)*	A _c (cpm)	B (cpm)
1	1	Quartz	750	2856	1.5	48,700	13.59	1.15
2	1	Quartz	1710	2756	3.0	51,500	31.64	2.3
3**†	1	Quartz						
4	1	Quartz	1663	2800				1.1
5†	1	Copper	1517	3100				0.8
6	1	Quartz	1690	2800	1.0	48,000	31.15	2.8
7	1	Quartz	532	2667	1.0	47,100	9.675	1.1
8	1	Copper	288	3067	0.75	46,000	6.017	0.8
9	7	Quartz	6840	2907	12.5	58,000	119.1	9.1
(Total)								
9A	1	Quartz	977	2907	1.9	47,000	17.5	1.7
9B	3	Quartz	2931	2907	5.3	52,000	50.2	3.6
9C	3	Quartz	2931	2907	5.3	52,000	51.4	3.8

*48-h measuring time; **Under construction; †Tritium counter

where A_c is the purity-corrected count rate in cpm, A_m the measured β -counting rate, and A_o the β -counting rate for standard recent $^{14}\text{CO}_2$. The correction terms contain the steep slope of the meson counting rate, and the β plateau slope for standard recent $^{14}\text{CO}_2$, as Figure 1 shows.

We make a similar correction for background (fossil anthracite) CO_2

$$B_c = B_m \left[1 - (N_z - N_{z_c}) \left(\frac{dV}{dN_\mu} \right)_{\max} \left(\frac{dN_B}{dV} \right) - (b - b_o) \frac{dN_B}{db} \right] \quad (2)$$

The final calculated activity is then determined by

$$A_{\text{final}} = [A_c - B_c] \frac{T}{T_o} \frac{p_o}{p} F \quad (3)$$

where b , p and T stand for barometer, pressure and temperature; F is the dilution factor used for small samples. For more details (also concerning counter construction), we refer to Grootes (1977) and Tans and Mook (1978).

The relations above obviously apply only to the radiocarbon proportional counters. Counters 4 and 5 are used for tritium with C_2H_6 as counting gas (Groeneveld 1977). Counter 3 is under construction and will use propane as counting gas.

ELECTRONICS

Figure 2 shows a schematic overview of the total counter setup. Each counter has a charge-sensitive preamplifier in the lead castle (close to the counter), connected to a controller unit. Also, the anticoincidence Geiger-Müller counters are connected to the controller unit. The preamplifier (model SP 2123 S) is a charge-integrating amplifier; the output voltage is proportional to the input charge and does not depend on the counter capacity. The controller unit (model SP226) is a 19-in rack containing an amplifier/discriminator model for the GM counter, an (anti-)coincidence module, a display unit and control buttons. With three adjustable discriminators (indicated as low, medium

controller collects the external parameters: barometer reading, and – for each counter system – pressure and temperature readings. This controller is also connected to the GPIB/IEEE bus. The controller units contain a G-64-based microprocessor (6809), which transfers the units basically into listen/talk state machines. G-64 is one of the standard buses for microprocessor-based systems. Devices (*e.g.*, 133, 134, . . . , 137; see below) are defined for communication with the display module, timer module, counter (channel) module, ADCs, *etc.* A special program is present in the 6809 processor; the main control program, TELBUIIS (running on the host PC), communicates with the controller units *via* these devices.

SOFTWARE

The counter setup is controlled by the program TELBUIIS, which is written in Turbo Pascal (version 5) (Borland 1989). The program controls data entry by means of the IEEE bus connection to the counter controller units; it is also used for offline analysis. Figure 3 shows the main menu. The main choices can be activated with function keys F1–F6. Measurements can be started with F1 or F2. For real measurements, F1 is used; the program is then linked to the counter electronics *via* IEEE. F2 can be used for testing purposes, and also on computers without an IEEE interface card; in this case, random counts are generated. For daily routine analysis, F3 is used. Measurement cycles (typically 100 min) can be excluded, proxy data, such as barometer reading and temperature, are averaged and a report is generated. Definitive results (such as averaging runs, age calculations, *etc.*) are usually generated offline with F4.

W E L C O M E		
to the C14/3H counter program – C.I.O. Groningen 1991		
F1	:	start the measurement – IEEE connected
F2	:	start the measurement – no IEEE connected
F3	:	calculations – one measurement run analysis
F4	:	calculations – definitive results
F5	:	edit measurement data
F6	:	edit counter constants
alt F1	:	change date and time
alt F2	:	routing output (printer/screen/disk)
alt F3	:	total restart program
alt F4	:	DOS commands
alt F5	:	info/help menu
alt F6	:	switch English/Dutch
alt F7	:	output to database
ESCAPE : exit program date : 10 5 1991 time : 13 23 58		

Fig. 3. Main menu for the data acquisition/analysis program, TELBUIIS

F5 and F6 are editing functions for measurement data (such as sample name, submitter, *etc.*) and counter constants, respectively. The keys, alt F1–alt F6 are useful options which can be accessed from the main menu. Alt F7 is reserved for output to other programs, such as the new data base (van der Plicht 1992), and will be installed in the new Groningen Radiocarbon Laboratory.

The program can further be explained using a (simplified) flow diagram (Fig. 4). After the measurement is started (F1, F2 from the main menu), the program asks which counters are connected. For these counters, two files are then called up, one containing the measurement data, and the other containing the counter constants. These files can be edited at this stage. The measurement data file contains administrative data such as GrN-number (for tritium: GT-number), sample number, sample name, submitter, *etc.* The counter constants data file contains background, recent activity, purity, correction factors, *etc.*

Next, the program's main loop, a continuous cycle, reading out the connected counters, is entered.

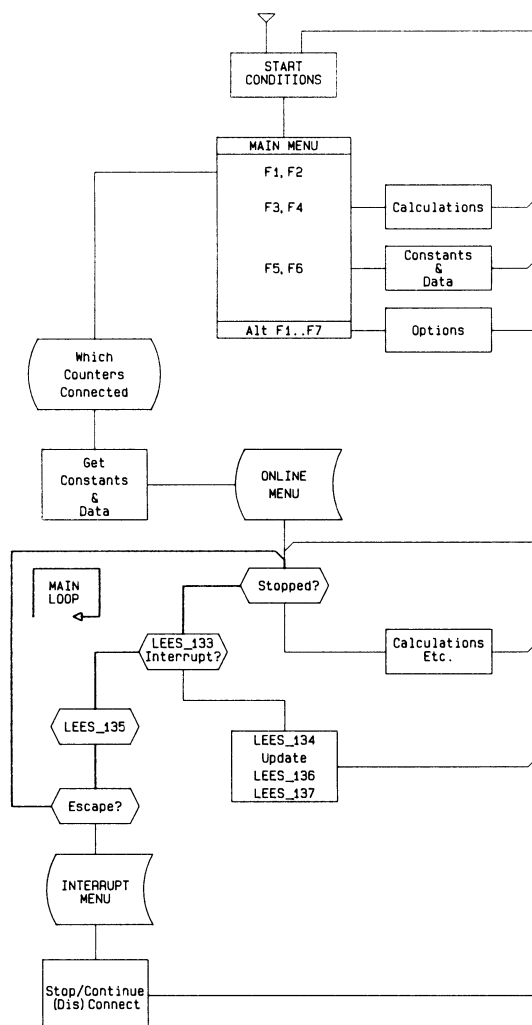


Fig. 4. Simplified flow diagram for the program, TELBUI5

The loop can be interrupted in only two ways: 1) one of the channels of the counter controller unit generates an interrupt, 2) from the program, TELBUI5, by hitting the escape key.

The hardware interrupt is generated when a measuring cycle (as a rule, 100 min) is finished. Device 133 (program LEES_133) checks for hardware interrupts and communicates which counter generated the interrupt. Next, the seven channels of the counter controller unit for the measurement cycle just finished will be read out by the computer (program LEES_134), as well as the measurement time (LEES_136) and the barometer-, pressure- and temperature-gauge readings (LEES_137). The program updates the data file on disk, and continues with the main loop.

In case of a software-generated interrupt, the program stops, and an interrupt menu gives the user five choices: continue the main loop (in case "escape" was used by accident), leave the program, restart the program, disconnect a counter from the program, or connect to the program a counter that was not active thus far.

During the main loop, *i.e.*, always operating when the counters are measuring, the program produces on the screen of the computer an online menu (Fig. 5), showing key data for every

counter, such as which counter is connected (indicated by status), GrN/GT number, Channel 0 (no. of beta counts), Channel 3 (purity counts) and measuring time per cycle (usually 100 min). This continuous readout of the (connected) counters is handled by Device 135 (program LEES_135) and has proven to be very useful as an overview for the performance of all 11 counters.

counter : 1 status : 1 GrN : 18885 chan. 0 : 7 chan. 3 : 198 meas.time: 100	counter : 5 status : 1 GT : 6697 chan. 0 : 208 chan. 3 : 235 meas.time: 100	counter : 9-A status : 1 GrN : 18546 chan. 0 : 89 chan. 3 : 82 meas.time: 100
counter : 2 status : 1 GrN : 18884 chan. 0 : 203 chan. 3 : 122 meas.time: 100	counter : 6 status : 1 GrN : 99999 chan. 0 : 173 chan. 3 : 212 meas.time: 100	counter : 9-B status : 1 GrN : 18546 chan. 0 : 240 chan. 3 : 199 meas.time: 100
counter : 3 status : 0 GrN : chan. 0 : chan. 3 : meas.time:	counter : 7 status : 1 GrN : 18889 chan. 0 : 148 chan. 3 : 159 meas.time: 100	counter : 9-C status : 1 GrN : 18546 chan. 0 : 63 chan. 3 : 127 meas.time: 100
counter : 4 status : 1 GT : 1111 chan. 0 : 43 chan. 3 : 90 meas.time: 100	counter : 8 status : 1 GrN : 11111 chan. 0 : 184 chan. 3 : 51 meas.time: 100	

date : 10 5 1991
 time : 13 30 28
 ESC for stopping

Fig. 5. Online screen during data acquisition

All data are recorded on disk, the file names keyed with the date the run was started and the counter number. The files are K_ddmmyy.TBx for counter constants, G_ddmmyy.TBx for the measurement data, A_ddmmyy.TBx for the file containing the raw data of the measurement cycles, B_ddmmyy.TBx the report (usually containing one full day of data) based on pre-analysis of the raw data, and D_ddmmyy.TBx the definitive results. In this notation, "ddmmyy" is the usual notation for day/month/year, and "x" corresponds to the counter number. The definitive results are usually calculated on an offline PC, using the same program, TELBUI. Several runs (*i.e.*, several files B_ddmmyy) can be averaged together. The final ages are calculated at this stage.

This setup of file bookkeeping allows automatic processing/reporting. Especially in a future network environment, the files with definitive results can be connected to other programs, such as the new Groningen radiocarbon database (van der Plicht 1992), calibration programs (van der Plicht & Mook 1989), administrative software or even programs from outside users.

REFERENCES

- Borland 1989 *Turbo Pascal*. Scotts Valley, California.
- Brenninkmeijer, C. A. M. and Mook, W. G. 1979 The effect of electronegative impurities on CO₂ proportional counting: An on-line purity test counter. In Berger, R. and Suess, H. E., eds., *Radiocarbon Dating*. Proceedings of the 9th International ¹⁴C Conference. Berkeley, University of California Press: 185-196.
- Groeneveld, D. J. 1977 (ms.) Tritium analysis of environmental water. Ph.D. dissertation, University of Groningen.
- Grootes, P. M. 1977 (ms.) Thermal diffusion, isotopic enrichment and radiocarbon dating beyond 50,000 years BP. Ph.D. dissertation, University of Groningen.
- Hut, G., Keyser, J. and Wijma, S. 1983 A multiple proportional ¹⁴C counter system for milligram-sized samples. In Stuiver M. and Kra, R. S., eds., *Proceedings of the 11th International ¹⁴C Conference*. *Radiocarbon* 25: 547-552.
- Mook, W. G. and Streurman, H. J. 1983 Physical and chemical aspects of radiocarbon dating. In Mook, W. G. and Waterbolk, H. T., eds., *Proceedings of the International Groningen Symposium ¹⁴C and Archaeology*. *PACT* 8: 31-55.
- Tans, P. P. and Mook, W. G. 1978 Design, construction and calibration of a high accuracy carbon-14 counting set up. *Radiocarbon* 21: 22-40
- van der Plicht, J. 1992 The new Groningen ¹⁴C data base. *Radiocarbon*, this issue.
- van der Plicht, J. and Mook, W. G. 1989 Calibration of Radiocarbon ages by computer. In Long, A. and Kra, R. S., eds., *Proceedings of the 13th International ¹⁴C Conference*. *Radiocarbon* 31(3): 805-816.